

**FIG. 1**

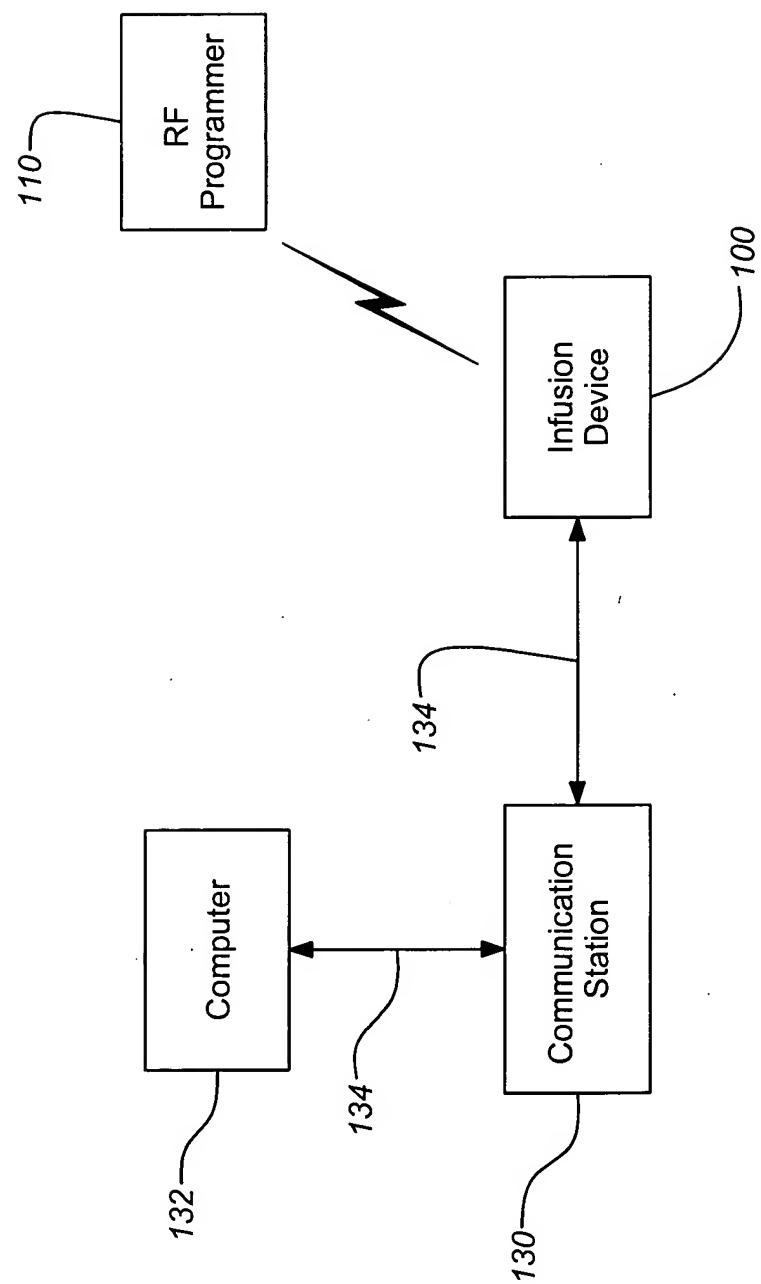


FIG. 2

Carbohydrate Ratio

302
304

Insulin Sensitivity

300
302

Auto Off	Off
Beep Volume	3
Audio Bolus	Off
Variable Bolus	On
Max Bolus	5.7 U
Max Basal	23 U/H
Time Display	24 Hr
Insulin Concentration	U100
Glucose Units	mg/DL
Remote Control	On
Alarm Mode	Both
Bolus Estimator	On
Target Blood Glucose	100 mg/dl
CHO Units	Exchange
Estimator Delay	1:30 (h:min)
Patterns	On
Current Delivery Pattern	Standard
Child Block	Off

FIG. 3A

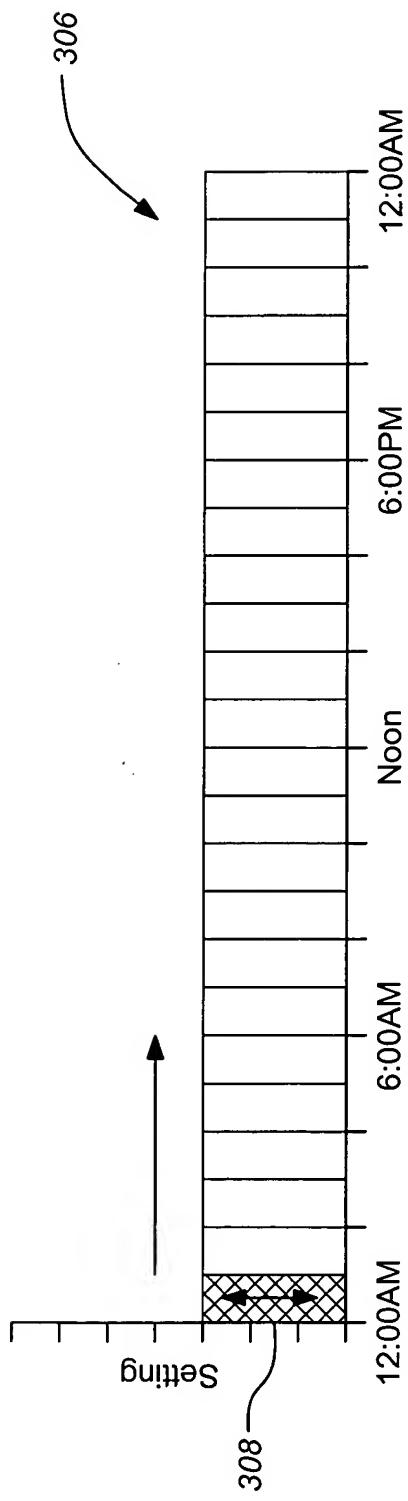


FIG. 3B

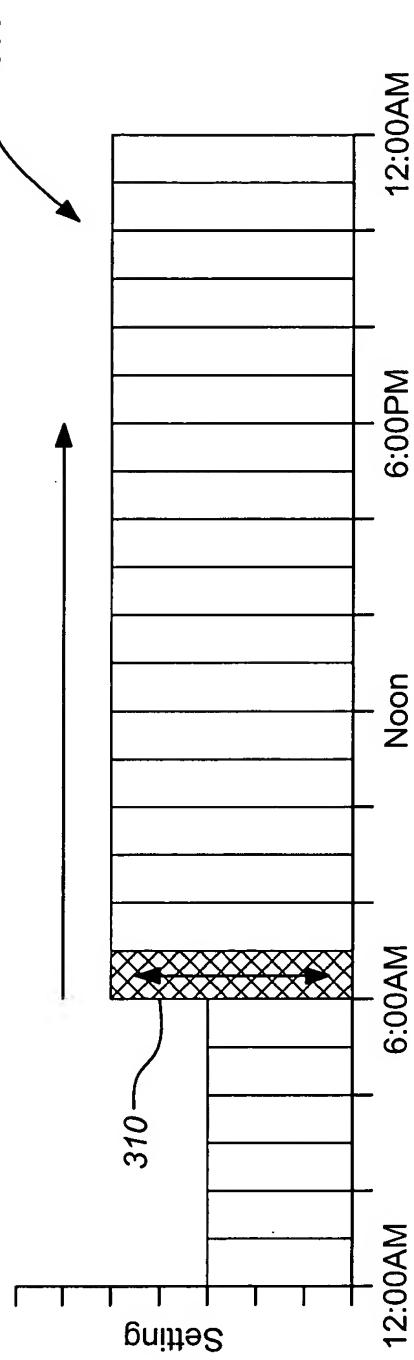


FIG. 3C

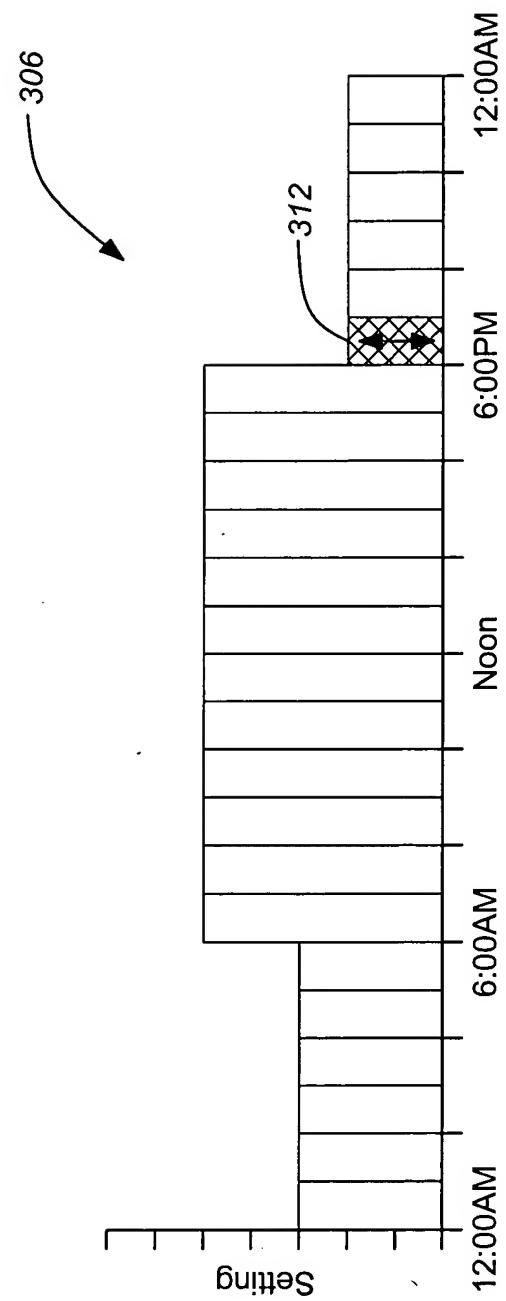


FIG. 3D

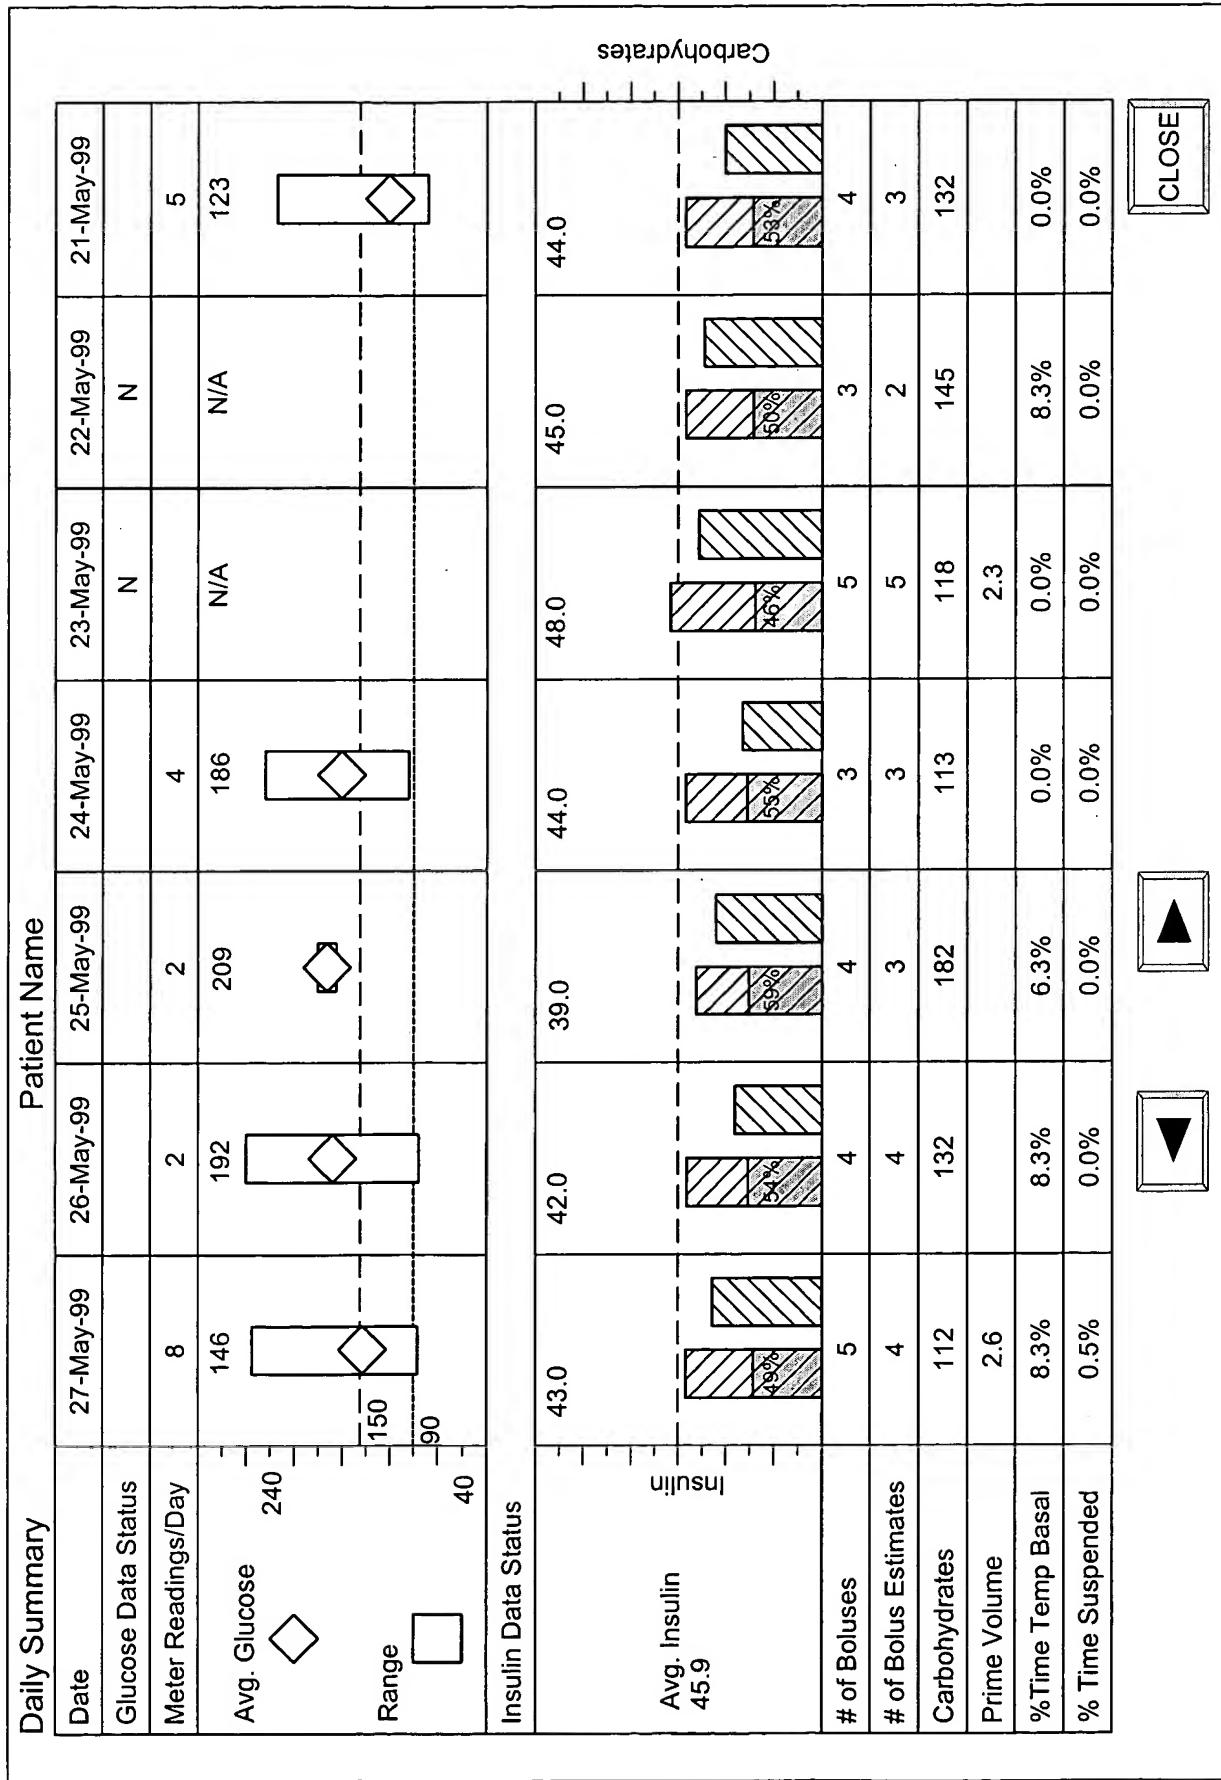
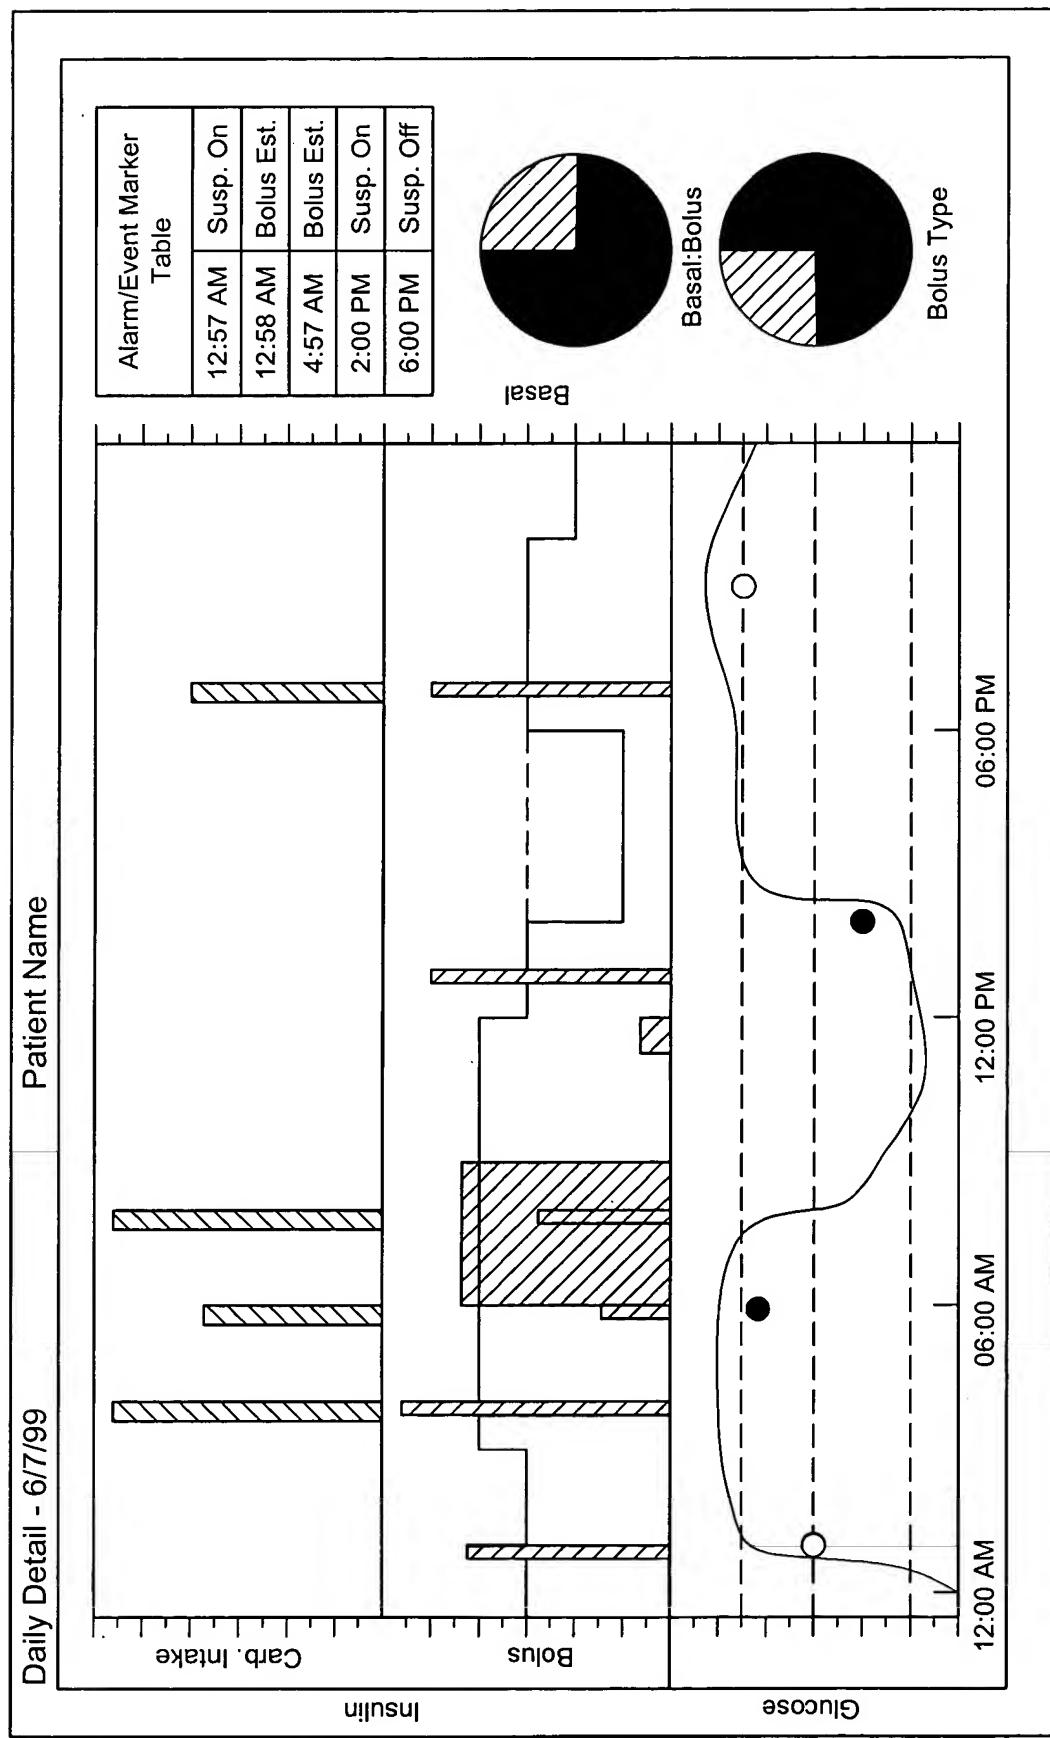


FIG. 4

FIG. 5



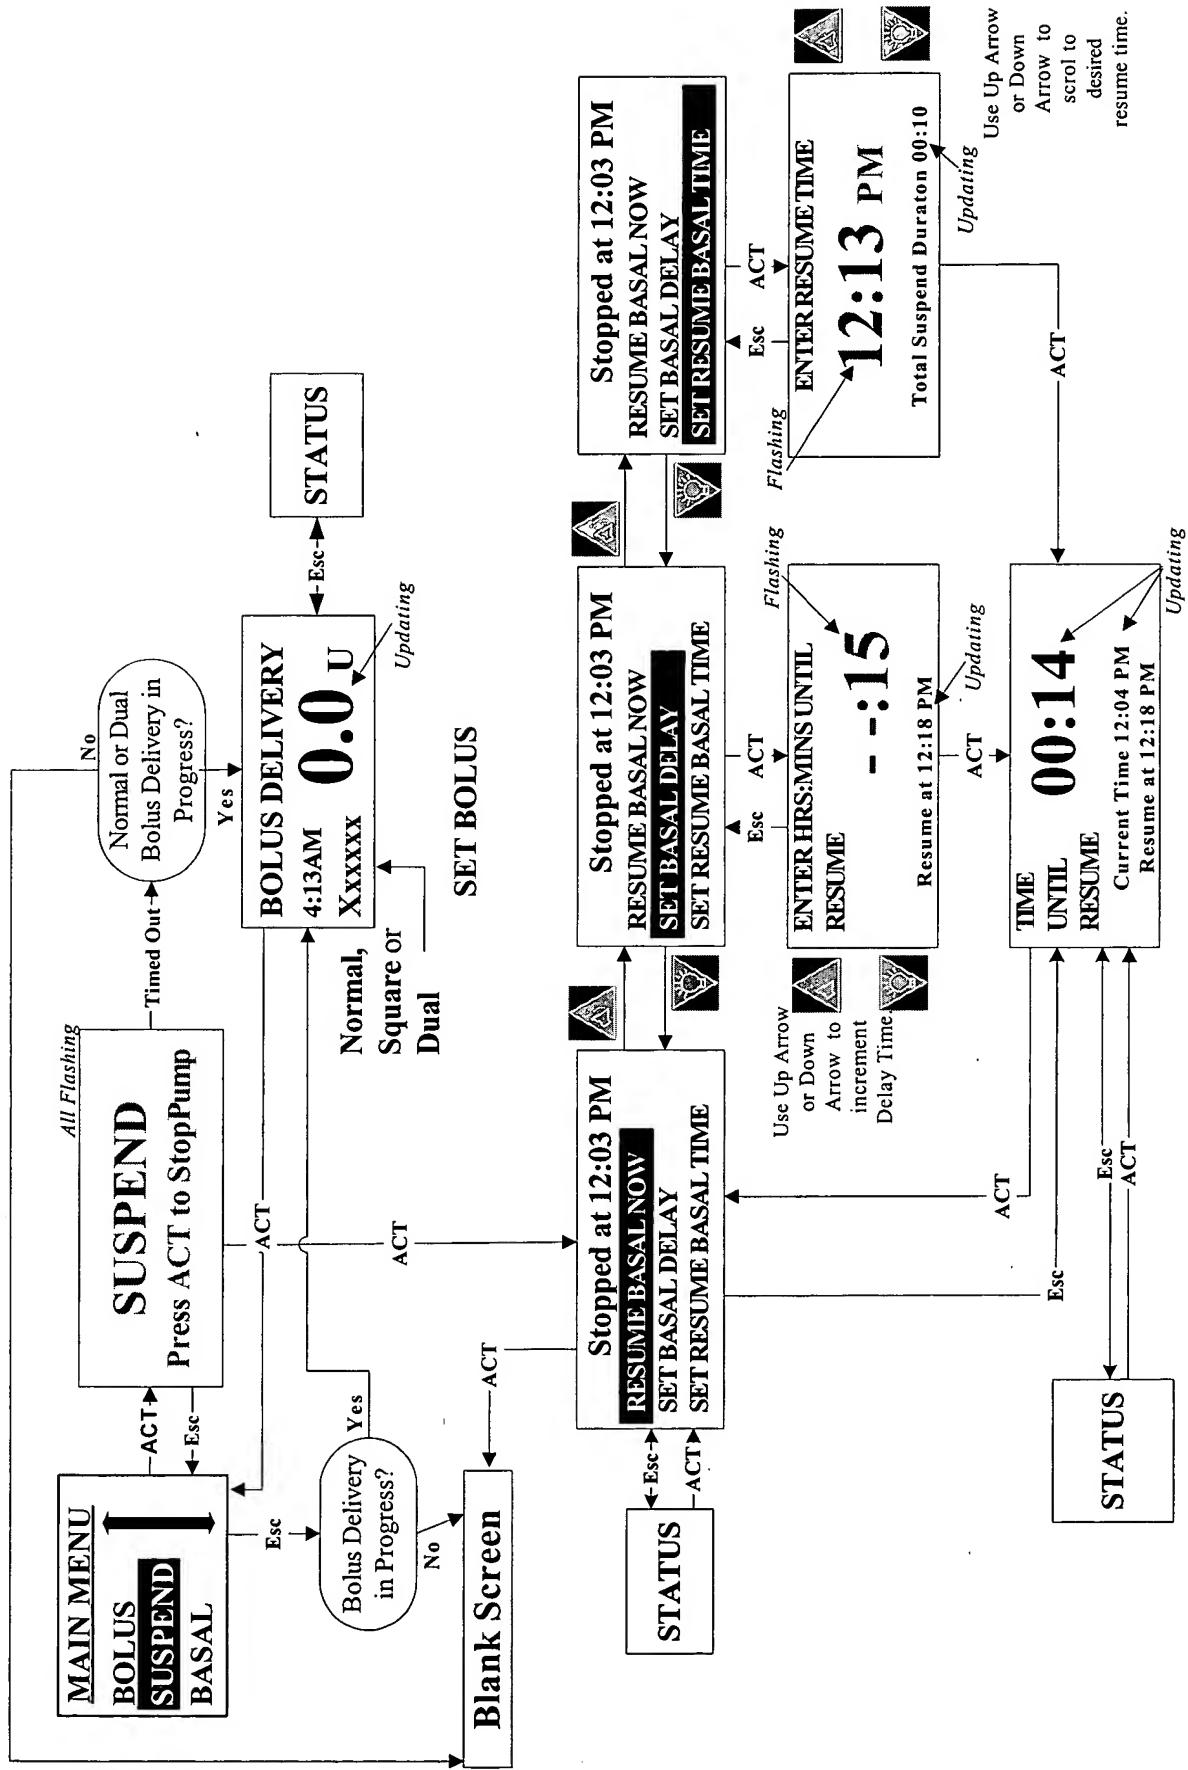
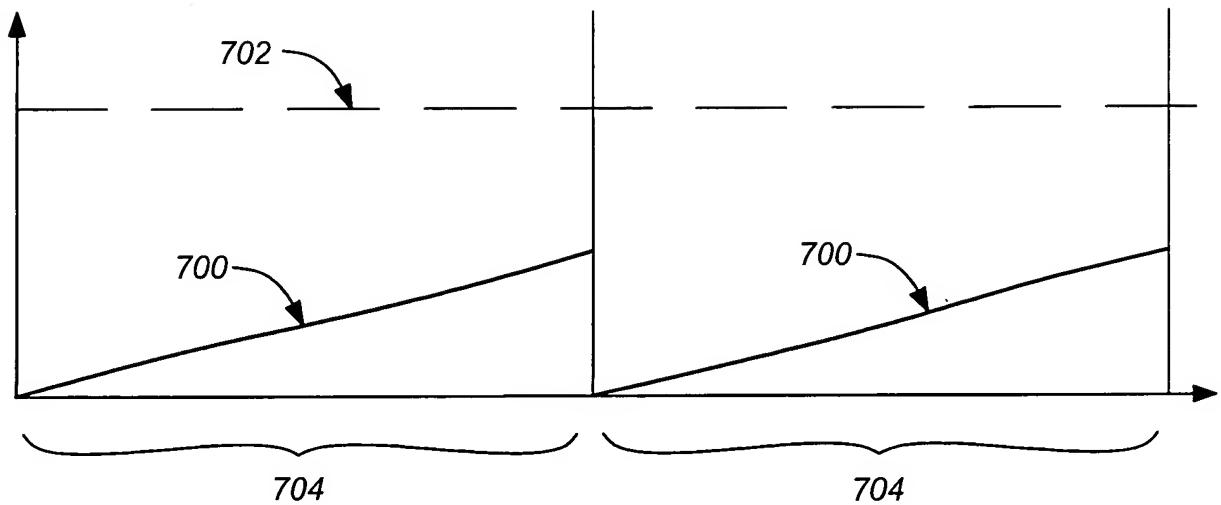
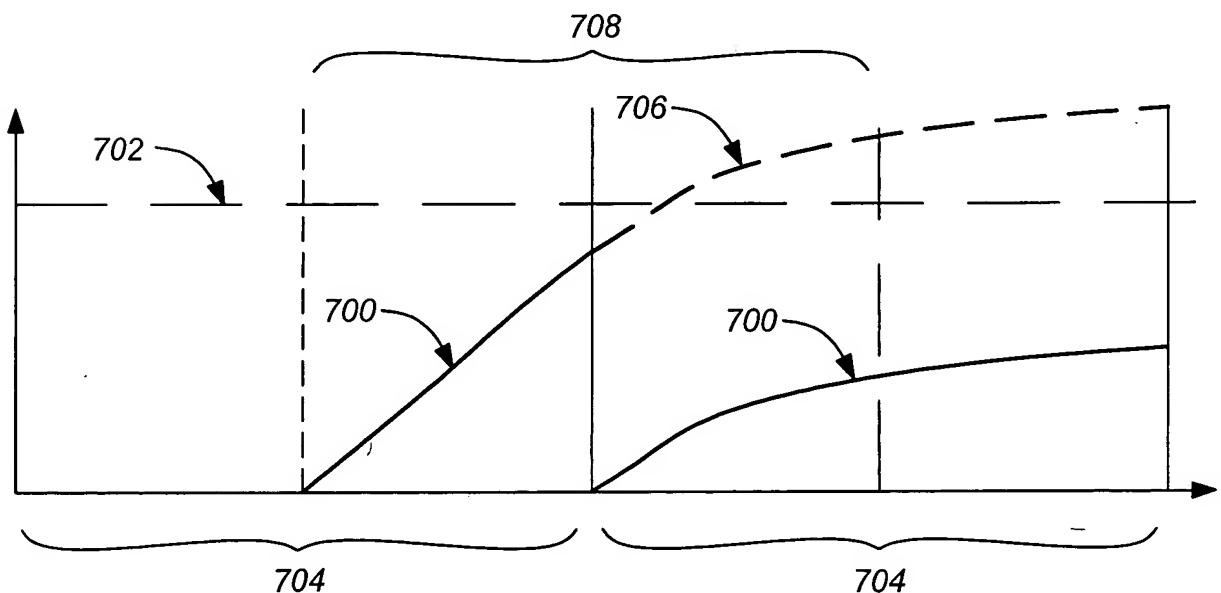


FIG. 6



*FIG. 7A*



*FIG. 7B*

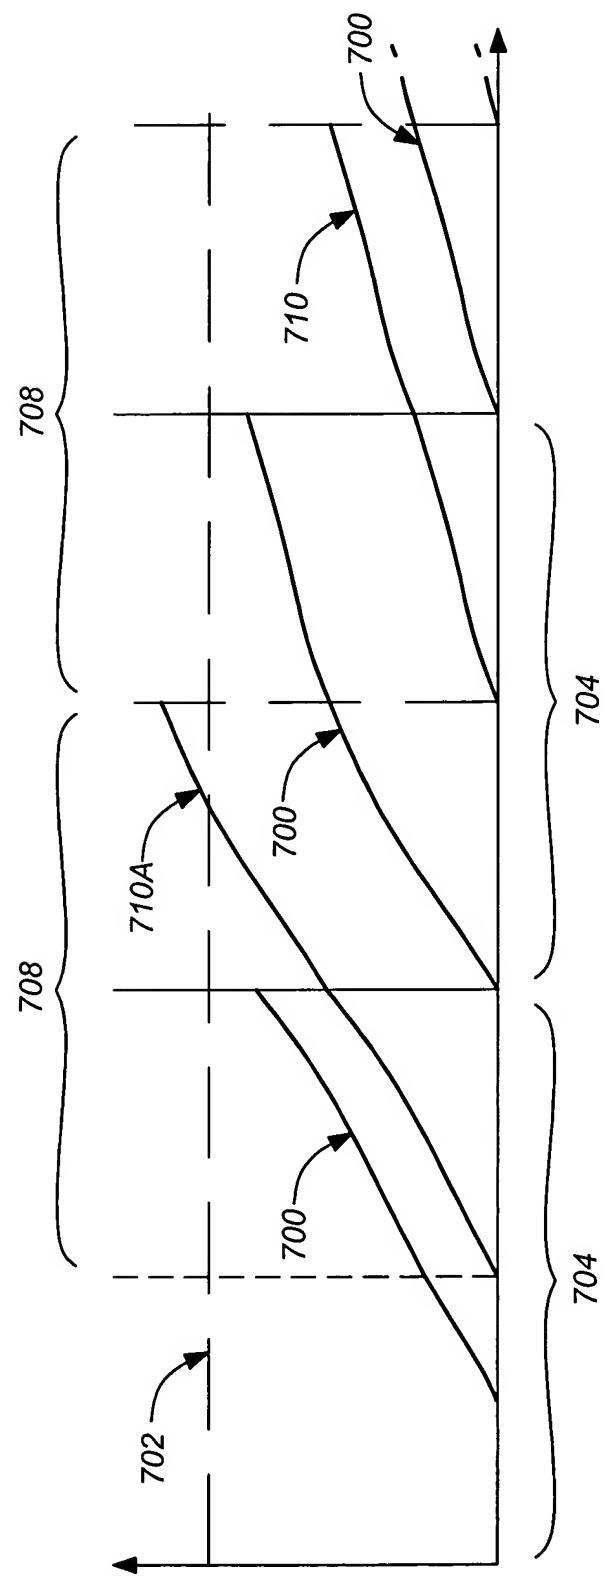


FIG. 7C